

Commentary

Cite this article: Limper U, Klaas L, Köhler M, *et al.* Limited utility of self-made oxygen generators assembled from everyday commodities during the COVID-19 pandemic. *Disaster Med Public Health Prep.* 17(e177), 1–4. doi: <https://doi.org/10.1017/dmp.2022.122>.


Keywords:

severe acute respiratory syndrome; oxygen supply; emergency preparedness

Corresponding author:

Ulrich Limper,
Email: Ulrich.limper@dlr.de.

Limited Utility of Self-made Oxygen Generators Assembled From Everyday Commodities During the COVID-19 Pandemic

Ulrich Limper MD^{1,2} , Lena Klaas MSc³, Markus Köhler⁴, Daniel Lichte PhD⁴, Nelson J Maldonado Samaniego MD⁵, Jose I Suarez MD⁶, Jens Jordan MD^{1,7} and Bernhard Hoffschmidt PhD^{4,8}

¹Institute of Aerospace Medicine, German Aerospace Center (DLR), Cologne, Germany; ²Department of Anesthesiology and Critical Care Medicine, Merheim Medical Center, Hospitals of Cologne, Witten/Herdecke University, Cologne, Germany; ³Institute of Future Fuels, German Aerospace Center (DLR), Cologne, Germany; ⁴Institute for the Protection of Terrestrial Infrastructures, German Aerospace Center (DLR), Sankt Augustin, Germany; ⁵Universidad San Francisco de Quito (USFQ), Quito, Ecuador; ⁶Division of Neurosciences Critical Care, Departments of Anesthesiology and Critical Care Medicine, Neurology, and Neurosurgery, The Johns Hopkins University School of Medicine, Baltimore, MD, USA; ⁷Chair of Aerospace Medicine, Faculty of Health, University of Cologne, Cologne, Germany and ⁸Institute of Solar Research, German Aerospace Center (DLR), Cologne, Germany

Abstract

The current COVID-19 pandemic has aggravated pre-existing oxygen supply gaps all over the world. In fact, oxygen shortages occurred in affluent areas with highly developed healthcare systems. The state-of-affairs created much suffering and resulted in potentially preventable deaths. Meanwhile, several international activities have been initiated to improve oxygen availability in the long-term by creating new networks of oxygen plants and supply channels. However, disasters such as the current pandemic may require rapid, autarkic oxygen production. Therefore, we determined whether oxygen resilience could conceivably be improved through self-made oxygen generators using material that is easily available even in remote areas. The team comprised engineers and physicians with hands-on experience in low- and middle-income countries. We constructed and tested self-made setups for water hydrolysis and membrane-based oxygen purification. We must conclude, however, that the massive amounts of oxygen patients with COVID-19 require cannot be reasonably met with such simple measures, which would require high efforts and hold potential risks.

Shortage of medical oxygen has been reported in the current COVID-19 pandemic in low, middle, and even high-income countries.^{1,2} In fact, shortness of oxygen supply in the face of a raging COVID-19 pandemic has been reported in California, jeopardizing medical care, hospitalizations, and patient discharges,^{3,4} in one of the strongest economies in the world. While high-income countries have the infrastructure to rapidly respond to changing oxygen demands, oxygen supply is a chronic challenge in low- and middle-income countries in Africa,⁵ Asia,⁶ and South America. The COVID-19 pandemic has made matters worse.^{7,8} The state-of-affairs is explained by purchasing costs, technical complexity, and the logistics required for transporting and storing medical oxygen.^{8,9} We reasoned that in truly catastrophic medical situations where increased oxygen needs cannot be reasonably met through conventional sources, oxygen could be generated through self-made generators using materials that are available in most countries. Therefore, we set out to determine the feasibility of building electrical hydrolysis and membrane-based oxygen generators with technology solely based on everyday commodities.

Existing technical solutions and their limitations in public health emergencies

The World Health Organization (WHO) and the United Nations Children's Fund published technical specifications and guidance for oxygen concentrator devices, stating that the produced medical gas should contain at least 82% oxygen and should be free of contaminants.¹⁰ Oxygen concentrators and oxygen cylinders are the 2 oxygen resources which are favored by the WHO to close oxygen gaps in less developed areas. Successful application of these guidelines requires reliable energy supply, gas distribution tubing, continuous technical maintenance, and patient respiratory monitoring. However, in disaster situations, multicomponent-based oxygen infrastructure may not be feasible.

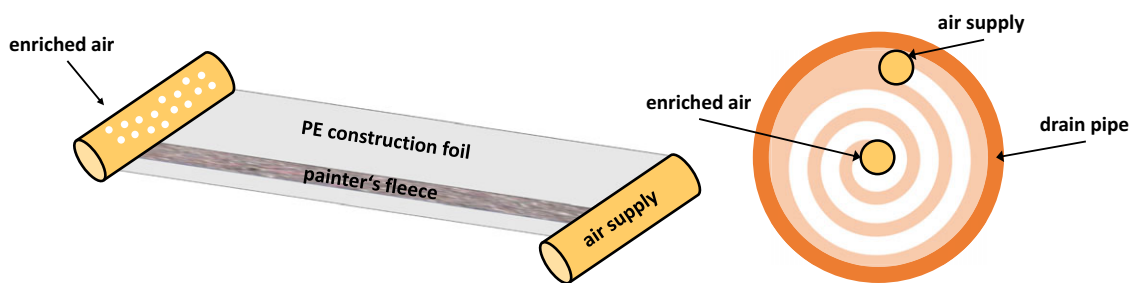


Figure 1. Schematic diagram of the assembled spiral-wound membrane oxygen generator. A: setup unreeled showing sandwiched polyethylene foil (PE) and painter's fleece; B: cross section of the self-made membrane reeled and encased in a plastic drainpipe.

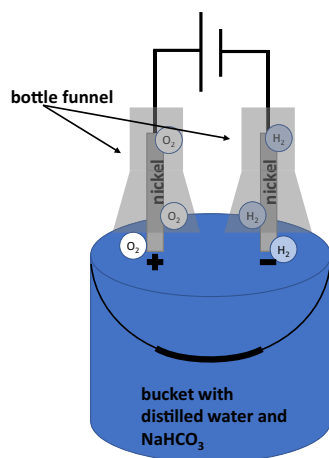


Figure 2. Schematic diagram of the assembled dialysis cell.

Theoretical considerations and testing of self-made devices

Membrane-based techniques for oxygen generation

Focusing on ambient temperature applications, polymeric membranes can be used for air separation. The functional principle is based on differences in diffusion velocities among gas molecules. Although oxygen molecules are only slightly smaller than nitrogen molecules, most membranes are more permeable to the former. The membrane separates high-pressure oxygen depleted and lower pressure oxygen enriched gas streams. The oxygen permeation is controlled by the oxygen diffusion rate through the membrane and the surface oxygen exchange kinetics, which requires a thin membrane with a large surface area. Selectivity of the membrane is defined by the ratio of the permeability of the gases. Due to a high membrane-area-to-volume ratio, the spiral wound membrane module and the hollow fiber membrane module are the most common membrane systems. Polymer membrane systems can reach purity levels of 60-80% of oxygen.¹¹ Continuous operation, compactness, and low operation costs are advantages of the systems.¹²

Practical testing of membrane-based oxygen generation

We thought that operation under ambient conditions would make this approach a good choice for self-made oxygen generation. Therefore, we constructed a membrane of polyethylene construction foil with a thickness of 80 μm and painter's fleece as a separator (Figure 1). We used pressure and heat applied via an iron as a heat sealer, to join 2 polyethylene foil layers air tightly together. The necessary air supply tubing consisted of a 6mm compressed air control line and the oxygen enriched outlet line of a cable protection pipe.

We wound up the membrane, and pushed it into a drainpipe with an outer protective layer of painter's fleece. We used an operating pressure of 1.5 bar, which is achieved by commercially available compressors. However, our device only achieved approximately 1% oxygen enrichment of air. The small surface area of 7.2 m^2 likely limited oxygen enrichment. Furthermore, the membrane was sensitive to mechanical damage through sand grains or other small objects such that a clean room would be required when assembling the device.

We therefore concluded that building a spiral wound out of workshop materials is unrealistic and cannot replace a fabricated spiral wound module, which guarantees a constant oxygen concentration.

Oxygen generation by electrical water hydrolysis

Water electrolysis is the process of decomposing water through electricity into its components, hydrogen, and oxygen. An electrolysis cell consists of 2 electrodes within an electrolyte which are connected by a power supply. The individual reactions at the electrodes are dependent on the characteristic of the electrolyte. The technically simplest approach is pure water electrolysis. The electrolysis cell consists of electrodes, electrolyte, and power supply. The electrode material influences the performance.¹³ Due to its stability and low corrosivity, nickel, and nickel-plated electrodes are preferable, although not available everywhere. Stainless steel, brass, or iron are inappropriate electrical conductors because of their fast decomposition and the formation of aggressive chemical compounds. Water electrolysis requires high voltages and produces an explosive gas, hydrogen.

Practical testing of electrical water hydrolysis

Water electrolysis was difficult to control with our self-made apparatus comprising of elementary materials such as buckets, plastic bottles, and nylon tight (Figure 2). We faced operational problems through the distance between anode and cathode. The wider separated the anode and cathode were, the more electrical power we needed. On the other side, short circuits happened when electrodes got in direct contact. To enable close electrode-contact without short circuits, we tested paper and nylon tight as insulators. However, paper was not suitable because of its flammability. Nylon tight prevented contact of the electrodes, yet they are permeable to the molecules. Eventually, the efficiency of our experimental setups ranged between 10 - 15% only.

Clean separation of the resulting gases (oxygen and hydrogen) could not be reached. Maintaining adequate safety without re-mixing the gases requires higher technical standards. For an electrolyte with a good ion conductivity, we used distilled water mixed with sodium bicarbonate.

We conclude that self-made electrolysis with the simplest means seems unsuitable in situations of disaster.

Oxygen generation through pressure-swing absorption

During pressure-swing-adsorption, differences in molecular absorption to surfaces are used to separate gases. The process works at ambient temperature and consists of 2 steps. First, a gas is trapped from a gas mixture by a bed of adsorbent materials at high pressures of about 3 - 6 bar. With increasing pressure, more molecules are adsorbed by the adsorbent material. For oxygen adsorption from air, the adsorbent material can be either zeolite or zeolite with additional metals.¹⁴ The material has a porous structure to increase the active surface area. When the adsorbent material is saturated, the pressure is reduced to ambient pressure for regeneration (pressure swings to low pressure). Molecules with the lowest affinity are being desorbed first. Since the affinity of the zeolite for nitrogen is higher than for oxygen, oxygen enriched air is produced. Gas purity of 90-95% can be achieved, however, reaching higher purity is challenging because zeolite has a similar affinity for O₂ and argon.¹⁴ To enable a quasi-continuous operation, 2 adsorbent columns are operated anti-cyclic.¹⁴

Practical testing of nitrogen tire gas generators for oxygen production

The absorption materials cannot be found among everyday commodities; however, they are part of commercial nitrogen tire gas generators, which are commonly available at car repair shops. Due to the complementary working method, an industrial nitrogen generator can easily be adjusted to serve as an oxygen generator. Therefore, the waste gas outlet is used. By adjusting the pressures, the oxygen content can be controlled and an oxygen concentration of 40% could be reached during our testing.

Discussion

Potentially beneficial effects of self-made oxygen must be balanced against potential harms. Oxygen of low quality (due to contamination with toxic gases or oil inhaled over a long period by patients with diseased lungs) could worsen outcomes. Furthermore, constructing and maintaining self-made oxygen devices would bind human resources of already strained health care systems. Construction and application of self-made oxygen supplies would only be justified if relevant amounts of oxygen-rich gases were harnessed. Furthermore, whether gas mixtures with only moderately enriched oxygen concentrations (30-80%) can improve medical outcome is unclear. Finally, oxygen purification is associated with increased risk of fire accidents.

Supplemental oxygen is 1 of the most important basic supplies for medical care. The current pandemic has once more revealed relevant oxygen supply gaps, particularly in low- and middle-income countries. The external support of critical oxygen infrastructure, by installation of industrial oxygen generators by foreign government organizations, has been shown to be fast and highly efficient under certain circumstances.⁸ However, for regions cut off from the outside world, autarkic solutions of improving oxygen generation would be essential.

In theory, oxygen generation is technically simple to achieve. In fact, we showed the feasibility to construct oxygen generators from everyday commodities. However, our observations suggest that none of the tested approaches provides enough oxygen that would justify the efforts and potential risks. Clearly, the massive amounts

of oxygen required in the COVID-19 pandemic cannot be met with such measures. Instead, efforts should be made to provide reliable, effective, and easy-to-maintain medical grade technology to countries in need.

Data availability statement. The data supporting the findings of this study are available within the article. No additional data available.

Acknowledgements. We are grateful to the team of the DLR Department of Sleep and Human Factors Research and the team of the European Transonic Wind tunnel (ETW) for their technical advice.

Author contributions. Ulrich Limper supervised the work from the standpoint of a medical doctor, contributed in the methodology, and wrote the original draft. Lena Klaas performed technical investigations and wrote the original draft. Markus Köhler worked on the methodology, performed investigations, reviewed, and edited the original draft. Daniel Lichte contributed to the methodology, performed investigations, reviewed, and edited the original draft. Nelson J Maldonado Samaniego supervised the work from a standpoint of a medical doctor from a low-income country, added to the methodology, reviewed, and edited the original draft. Jose I Suarez supervised the work, reviewed, and edited the original draft. Jens Jordan (guarantor) contributed to the conceptualization of the study, supervised the work, reviewed, edited the original draft, and acquired funding. Bernhard Hoffschmidt (guarantor) contributed to the conceptualization and methodology, supervised the formal analysis, acquired funding, reviewed, and edited the original draft.

Funding statement. This study was supported by the programmatic funding of the German Aerospace Center (DLR). Ulrich Limper received funding from the internal grant program (project IFF 2020-26) of the Faculty of Health at Witten/Herdecke University, Germany, during preparation of this work.

Competing interests. Ulrich Limper, Lena Klaus, Markus Köhler, Daniel Lichte, Jens Jordan, Bernhard Hoffschmidt, and Nelson J Maldonado have nothing to disclose related to this project. Jose I Suarez is the Chair for the DSMB for the INTREPID Study supported by BARD. Dr Suarez has received no monetary compensation for this activity. He is also a member of the Clinical Events Committee for the REACT Study funded by IDORSIA. Dr Suarez has received less than US\$10000 for this activity.

Ethical standards. No patients were involved.

References

1. Tyrrell CSB, Mytton OT, Gentry SV, *et al.* Managing intensive care admissions when there are not enough beds during the COVID-19 pandemic: a systematic review. *Thorax*. 2021;76(3):302-312. doi: [10.1136/thoraxjnl-2020-215518](https://doi.org/10.1136/thoraxjnl-2020-215518)
2. Kliff S, Satariano A, Silver-Greenberg J, Kulish N. There aren't enough ventilators to cope with the Coronavirus. *The New York Times*. Updated March 26, 2020. <https://www.nytimes.com/2020/03/18/business/coronavirus-ventilator-shortage.html>
3. Patil A. As the coronavirus rages in California, L.A. medics are told to ration oxygen. *The New York Times*. January 5, 2021.
4. Devereaux AV, Backer H, Salami A, *et al.* Oxygen and ventilator logistics during California's COVID-19 surge: when oxygen becomes a scarce resource [published online ahead of print, 2021 Aug 16]. *Disaster Med Public Health Prep*. 2021;1-7. doi: [10.1017/dmp.2021.267](https://doi.org/10.1017/dmp.2021.267)
5. Mangipudi S, Leather A, Seedat A, Davies J. Oxygen availability in sub-Saharan African countries: a call for data to inform service delivery. *The Lancet Global health*. 2020;8:e1123-e1124. doi: [10.1016/s2214-109x\(20\)30298-9](https://doi.org/10.1016/s2214-109x(20)30298-9)
6. Gettleman J. The night the oxygen ran out in an Indian hospital. *The New York Times*. August 17, 2017.

7. **McNeil Jr DG.** A simple way to save lives as Covid-19 hits poorer nations. *The New York Times*. Updated Septemeber 30, 2020. <https://www.nytimes.com/2020/06/23/health/coronavirus-oxygen-africa.html>
8. **Stroffolini G, Cortellaro F, Raviolo M, Tommasoni N, Gupta Kumar M, Marotta C.** Improving oxygen capacity at ITBP Referral Hospital during the second wave of COVID-19 infections in Greater Noida, India: an operative targeted intervention [published online ahead of print, 2021 Dec 23]. *Disaster Med Public Health Prep.* 2021;1-16. doi: [10.1017/dmp.2021.372](https://doi.org/10.1017/dmp.2021.372)
9. **Stein F, Perry M, Banda G, Woolhouse M, Mutapi, F.** Oxygen provision to fight COVID-19 in sub-Saharan Africa. *BMJ Global Health.* 2020;5:e002786. doi: [10.1136/bmjgh-2020-002786](https://doi.org/10.1136/bmjgh-2020-002786)
10. **World Health, Organization, United Nations Children's Fund.** *WHO-UNICEF technical specifications and guidance for oxygen therapy devices.* 2019;viii:149.
11. **Murali RS, Sankarshana T, Sridhar S.** Air separation by polymer-based membrane technology. *Sep Purif Rev.* 2013;42:130-186. doi: [10.1080/15422119.2012.686000](https://doi.org/10.1080/15422119.2012.686000)
12. **Robeson LM.** Polymer membranes for gas separation. *Curr Opin Solid State Mater Sci.* 1999;4:549-552. [https://doi.org/10.1016/S1359-0286\(00\)00014-0](https://doi.org/10.1016/S1359-0286(00)00014-0)
13. **Chakik FE, Kaddami M, Mikou M.** Effect of operating parameters on hydrogen production by electrolysis of water. *Int J Hydrog.* 2017;42:25550-25557. <https://doi.org/10.1016/j.ijhydene.2017.07.015>
14. **Santos JC, Cruz P, Regala T, Magalhães FD, Mendes A.** High-purity oxygen production by pressure swing adsorption. *Ind Eng Chem Res.* 2007;46:591-599. doi: [10.1021/ie060400g](https://doi.org/10.1021/ie060400g)