

INFECTION CONTROL AND HOSPITAL EPIDEMIOLOGY[®]

EDITORIAL

- Classification of the Surgical Wound: A Time for Reassessment and Simplification 253
RONALD LEE NICHOLS, MD

ORIGINAL ARTICLES

- Validation of Surgical Wound Classification in the Operating Room 255
DENISE M. CARDO, MD; PAMELA S. FALK, MPH; C. GLEN MAYHALL, MD

- Oxacillin- and Quinolone-Resistant *Staphylococcus aureus* in Sao Paulo, Brazil: A Multicenter Molecular Epidemiology Study 260
HELIO S. SADER, MD; ANTONIO C. PIGNATARI, MD; RICHARD J. HOLLIS, MS; IVANI LEME, MS; RONALD N. JONES, MD

- A Cluster of Surgical Wound Infections due to Unrelated Strains of Group A Streptococci 265
E.B. JAMIESON, MD, FRCPC; K. GREEN, RN, CIC; D.E. LOW, MD, FRCPC
A.E. SIMOR, MD, FRCPC; C. GOLDMAN, BSCN; J. NG, ART; A. MCGEER, MD, FRCPC

- Brucellosis Among Hospital Employees in Saudi Arabia 268
FRANK W. KIEL, MD; M. YOUSUF KHAN, MD

READERS' FORUM

- Wash Hands, Disinfect Hands, or Don't Touch? Which, When, and Why? 273
ALLAN PERCEVAL, MSC, MASM

PRODUCT COMMENTARY

- Efficacy of Chemical Sterilants/Disinfectants: Is There a Light at the End of the Tunnel? 276
INGE GUREVICH, RN, MA

BEYOND INFECTION CONTROL: THE NEW HOSPITAL EPIDEMIOLOGY

- Agency for Healthcare Policy and Research 279
BRYAN P. SIMMONS, MD; STEPHEN B. KRITCHEVSKY, PHD

TOPICS IN CLINICAL MICROBIOLOGY

- Rhodococcus* 282
ROBERT D. WALSK, MD, PHD; PAUL E. SCHOCH, PHD; BURKE A. CUNHA, MD

LETTERS TO THE EDITOR


- Cost Improvement Through Prudent Infection Control in a Brazilian Hospital 250
HEIKO GEISS, MD

- Universal Precautions Kit 252
PHYLLIS A. KEPHART, MD; KATHLEEN L. ROMAN, RN, BSN-ICN; DEBORAH M. MYERS

- MEDICAL NEWS 289

- SHEA NEWS 299

Dream Machine.

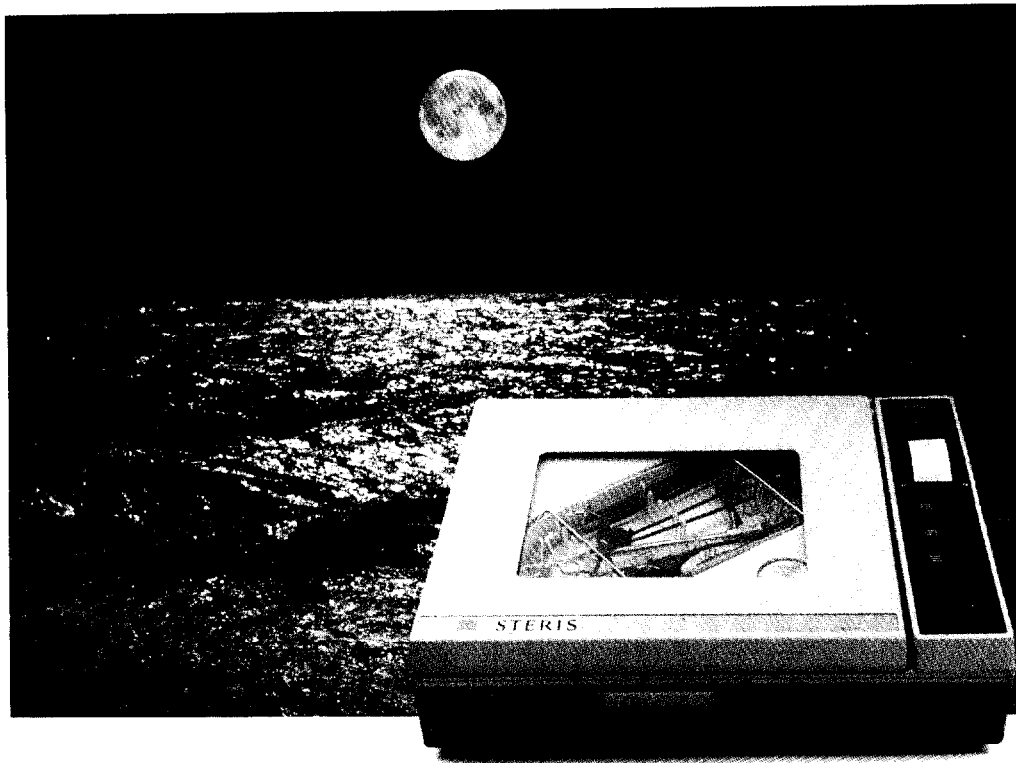

**Rapid, Safe,
Sterile Processing
Was Once
Just A Dream**

● STERIS SYSTEM 1™ has made the dream of rapid and safe sterile processing a reality.

STERIS SYSTEM 1 is the proven, low temperature sterile processing system for immersible surgical and diagnostic devices. Even delicate, heat sensitive scopes, cameras, instruments, and accessories can be safely sterilized in less than 30 minutes-Just In Time for each patient procedure. ●

STERIS SYSTEM 1 also provides peace of mind. There are no toxic fumes, and no disposal restrictions to lose sleep over. ● And liquid processing means that your devices can be sterilized without the drying and wrapping which are required with gaseous systems.

Write or call us today to learn why thousands of health professionals rest assured with the rapid and safe sterile processing of STERIS SYSTEM 1. ○

The STERIS PROCESS™
The Proven Process
Just In Time

STERIS®



Answers To Commonly Asked Questions About the STERIS PROCESS™

LIQUID STERILE PROCESSING

Q. How does liquid sterile processing compare to other methods? Q. How is the STERIS PROCESS different from other liquid processes?

A. Regardless of the sterilization process, the item to be sterilized must be clean to ensure effective sterilization. The cleaning process is universally performed by washing an item with water. Gas sterilization technologies, such as EtO and vaporized hydrogen peroxide, require that an item be completely dry before it is exposed to the sterilization process. This adds time, difficulty, and uncertainty—all negatives when a health professional is rushing to get ready to treat the next patient.

Since the STERIS PROCESS uses a liquid sterilant, it is equally effective on wet or dry items. This allows processing of items immediately after pre-cleaning without additional preparation. And since the STERIS PROCESS does not require wrapping and unwrapping of items, it eliminates many processing steps which are typically performed with gaseous systems, and allows sterilization with optimum efficiency and efficacy.

Liquid processing offers many other advantages as well. Liquid solutions are more easily directed than gases. This is especially important when processing sophisticated devices such as lumened endoscopes, which pose a challenge to chemical sterilization technologies. In addition, sterile processing with STERIS SYSTEM 1™ allows the user to see the gentle agitation of the liquid solution in action, without having to rely on complex monitoring systems to ensure that the sterilizing agents are present.

A. The STERIS PROCESS uses STERIS 20™, a powerful chemical sterilant with a high degree of materials compatibility. The STERIS 20 formulation includes the active biocidal agent, peracetic acid, in combination with a proven chemical protection system. The ability to deliver anti-corrosives to all surfaces of a device is an important advantage of a liquid system.

The STERIS PROCESS is used in STERIS SYSTEM 1—a complete sterile processing system. SYSTEM 1 provides automated and documented sterile processing in less than 30 minutes, so sterile devices are available Just In Time for each patient procedure.

Q. How is the STERIS 20 solution different from other solutions, like glutaraldehyde?

A. Glutaraldehyde solutions are typically used only to disinfect, not sterilize. These solutions are normally reused, allowing contamination and/or dilution. Unlike STERIS 20, glutaraldehyde cross links proteins, and therefore, can affix organic material to instrument surfaces. The STERIS 20 formulation, along with the directed flow of SYSTEM 1, makes the STERIS PROCESS more effective at reaching contaminated surfaces.

STERIS 20 does not have the same hazardous waste and worker exposure considerations as glutaraldehyde. The STERIS 20 use dilution is non-toxic and safely disposed in an ordinary drain during the standard processing cycle. In fact, it has passed the stringent fish toxicity tests required by the U.S. EPA and the State of California.

STERIS Corporation develops, manufactures, and markets sterile processing and infection prevention systems for the worldwide healthcare market. STERIS® is committed to providing products which improve patient and worker safety. If you would like more information about STERIS or STERIS SYSTEM 1, please write or call us at 1-800-JIT-4-USE (1-800-548-4873).

Paid Advertisement





VACUTAINER[®] BRAND Safety-Lok[™] BLOOD COLLECTION SET

Ease of use

because safety and ease of use
are built into the design.

Ease of mind...

because your focus
should be on your patient



For use in accordance with the
OSHA Bloodborne Pathogens Standards.
Please refer to package insert for
caution statement before use.

For more information, please call
1-800-631-0174.

**BECTON
DICKINSON**

Becton Dickinson VACUTAINER Systems, Franklin Lakes, New Jersey, 07417-1885
VACUTAINER and Safety-Lok are trademarks of Becton Dickinson and Company.
US Patent Number 5,120,320

© 1993

**Meets OSHA guidelines:
Engineered for safety
New**

INFECTION CONTROL AND HOSPITAL EPIDEMIOLOGYTM

CONTENTS

EDITORIAL

- Classification of the Surgical Wound: A Time for Reassessment and Simplification **253**
RONALD LEE NICHOLS, MD

ORIGINAL ARTICLES

- Validation of Surgical Wound Classification in the Operating Room **255**
DENISE M. CARDO, MD; PAMELA S. FALK, MPH; C. GLEN MAYHALL, MD
- Oxacillin- and Quinolone-Resistant *Staphylococcus aureus* in Sao Paulo, Brazil: A Multicenter Molecular Epidemiology Study **260**
HELIO S. SADER, MD; ANTONIO C. PIGNATARI, MD; RICHARD J. HOLLIS, MS; IVANI LEME, MS; RONALD N. JONES, MD
- A Cluster of Surgical Wound Infections due to Unrelated Strains of Group A Streptococci **265**
E.B. JAMIESON, MD, FRCPC; K. GREEN, RN, CIC; D.E. LOW, MD, FRCPC; A.E. SIMOR, MD, FRCPC; C. GOLDMAN, BSCN; J. NG, ART; A. MCGREER, MD, FRCPC
- Brucellosis Among Hospital Employees in Saudi Arabia **268**
FRANK W. KIEL, MD; M. YOUSUF KHAN, MD

READERS' FORUM

- Wash Hands, Disinfect Hands, or Don't Touch? Which, When, and Why? **273**
ALLAN PERCEVAL, MSc, MASM

PRODUCT COMMENTARY

- Efficacy of Chemical Sterilants/Disinfectants: Is There a Light at the End of the Tunnel? **276**
INGE GUREVICH, RN, MA

BEYOND INFECTION CONTROL: THE NEW HOSPITAL EPIDEMIOLOGY

- Agency for Healthcare Policy and Research **279**
BRYAN P. SIMMONS, MD; STEPHEN B. KRITCHEVSKY, PHD

TOPICS IN CLINICAL MICROBIOLOGY

- Rhodococcus* **282**
ROBERT D. WALSH, MD, PhD; PAUL E. SCHOCH, PhD; BURKE A. CUNHA, MD

DEPARTMENTS

- Letters to the Editor **250**
- Medical News **289**
- Calendar of Events **296**
- SHEA News **299**

THE PUBLICATION OF ADVERTISING IN THE JOURNAL DOES NOT CONSTITUTE ANY GUARANTEE OR ENDORSEMENT BY THE SOCIETY FOR HOSPITAL EPIDEMIOLOGY OF AMERICA OR SLACK INCORPORATED OF THE ADVERTISED PRODUCT OR SERVICE OR OF CLAIMS MADE BY THE ADVERTISER. THE PUBLICATION OF ARTICLES AND OTHER EDITORIAL MATERIAL IN THE JOURNAL DOES NOT NECESSARILY REPRESENT THE POLICY RECOMMENDATIONS OR ENDORSEMENT BY THE SOCIETY.

PUBLISHER: Infection Control and Hospital Epidemiology (ISSN-0899-823X, Canadian GST#129780466) is published exclusively by SLACK Incorporated 12 times a year. Address: 6900 Grove Rd., Thorofare, NJ 08086. Telephone: (609) 848-1000.

COPYRIGHT 1993 The Society for Hospital Epidemiology of America, Inc., and SLACK Incorporated. All rights reserved. No part of this publication may be reproduced without written permission from the publisher. Printed in the USA.

SUBSCRIPTIONS: Requests should be addressed to the publisher (except Japan). In Japan, contact Woodbell Incorporated, 4-22-11, Kitakasai, Edogawaku, Tokyo 134, Japan. Subscription rates in the United States and possessions: Individual: One year-\$80.00; Two years-\$115.00; Three years-\$145.00; Institutional: One year-\$90.00; Two year-\$130.00; Three years-\$170.00. Fellows: \$20 per year with proof of training status. Canada: \$18.00 additional each year plus 7% for Canadian Goods & Services tax; all other countries: \$36.00 additional each year. Single copies of current issues may be obtained for \$15.00, United States and possessions; \$20.00 all other countries.

REPRINTS: All requests to reprint or use material published herein should be addressed to Lester Robeson, SLACK Incorporated, 6900 Grove Rd., Thorofare, NJ 08086. For reprint orders and prices, contact Lester Robeson at (609) 848-1000. Authorization to photocopy items for internal or personal use, or the internal or personal use of specific clients, is granted by SLACK Incorporated, provided that the base fee of \$1.00 per copy, plus \$15 per page is paid directly to Copyright Clearance Center, 27 Congress St., Salem, MA 01970. This consent does not extend to other kinds of copying, such as for general distribution, resale, advertising and promotional purposes, or for creating new collective works.

CHANGE OF ADDRESS: Notice should be sent to the publisher six weeks in advance of effective date. Include old and new addresses with zip codes. The publisher cannot accept responsibility for undelivered copies. Second-class postage is paid at Thorofare, New Jersey 08086, and additional entry points. **POSTMASTER:** Send address changes to SLACK Incorporated, 6900 Grove Rd., Thorofare, NJ 08086.

INFECTION CONTROL AND HOSPITAL EPIDEMIOLOGY is listed in Index Medicus, Current Contents—Clinical Practice, Hospital Literature Index, Cumulative Index to Nursing & Allied Health Literature, Nursing Abstracts, and Laboratory Performance Information Exchange System.

EDITORIAL OFFICES

Vanderbilt University School of Medicine
 A-1131 Medical Center North
 Nashville, TN 37232-2637
 (615) 343-1095; (615) 343-1882 (FAX)
 Email: iche@mcmail.vanderbilt.edu

EDITOR

Michael D. Decker, MD, MPH

MANAGING EDITOR

Susan Cantrell

STATISTICAL EDITOR

Beverly G. Mellen, PhD

SENIOR ASSOCIATE EDITORS

C. Glen Mayhall, MD

Gina Pugliese, RN, MS

William Schaffner, MD

ASSOCIATE EDITORS

Donald A. Goldmann, MD

Didier Pittet, MD, MS

Andreas Widmer, MD, MS

SECTION EDITORS**Beyond Infection Control:****The New Hospital Epidemiology**

Bryan P. Simmons, MD

Stephen B. Kritchevsky, PhD

Memphis, Tennessee

Wing Hong Seto, MD

Hong Kong

Disinfection and Sterilization

William A. Rutala, PhD, MPH

Chapel Hill, North Carolina

Emerging Infectious Diseases

Larry J. Strausbaugh, MD

Portland, Oregon

Robert W. Pinner, MD

Atlanta, Georgia

From the Laboratory

Marcus Zervos, MD

Royal Oak, Michigan

Fred C. Tenover, PhD

Atlanta, Georgia

Information Management

John A. Sellick, DO

Buffalo, New York

The International Perspective

Mary D. Nettleman, MD, MS

Richmond, Virginia

Issues in Surgery

James T. Lee, MD, PhD

St. Paul, Minnesota

Medical News

Gina Pugliese, RN, MS

Chicago, Illinois

Martin S. Favero, PhD

Irvine, California

Practical Healthcare Epidemiology

Loreen A. Herwaldt, MD

Iowa City, Iowa

SHEA News

Murray D. Batt, MD

Clarksburg, West Virginia

Statistics for Hospital Epidemiology

David Birnbaum, PhD, MPH

Sidney, British Columbia, Canada

Topics in Long-Term Care

Philip W. Smith, MD

Omaha, Nebraska

Topics in Occupational Medicine

David Weber, MD, MPH

Chapel Hill, North Carolina

INFECTION CONTROL AND HOSPITAL EPIDEMIOLOGY[®]

EDITORIAL ADVISORY BOARD

- Jacques F. Acar, MD Paris, France
 J. Wesley Alexander, MD Cincinnati, Ohio
 Paul Arnow, MD Chicago, Illinois
 Graham A.J. Ayliffe, MD Birmingham, United Kingdom
 Neil L. Barg, MD Yakima, Washington
 Elizabeth Ann Bolyard, RN, MPH, CIC Atlanta, Georgia
 John M. Boyce, MD Providence, Rhode Island
 Professor Dr. Ilja Braveny Munich, Federal Republic of Germany
 Charles Bryan, MD Columbia, South Carolina
 Christian Brun-Buisson, MD Creteil, France
 Donald E. Craven, MD Boston, Massachusetts
 Sue Crow, MSN, RN, CIC Shreveport, Louisiana
 Franz Daschner, MD Freiburg, Federal Republic of Germany
 Leigh G. Donowitz, MD Charlottesville, Virginia
 Charles E. Edmiston, Jr., PhD Milwaukee, Wisconsin
 Theodore C. Eickhoff, MD Denver, Colorado
 Bruce Farber, MD Manhasset, New York
 Victoria J. Fraser, MD St. Louis, Missouri
 Peter C. Fuchs, MD, PhD Black Butte, Oregon
 Richard A. Garibaldi, MD Farmington, Connecticut
 Velvl Greene, PhD, MPH Beer Sheva, Israel
 Robert Gaynes, MD Atlanta, Georgia
 David W. Gregory, MD Nashville, Tennessee
 David K. Henderson, MD Bethesda, Maryland
 Peter N.R. Heseltine, MD Los Angeles, California
 Karen Hoffmann, RN, CIC, MS Chapel Hill, North Carolina
 Marguerite McMillan Jackson, RN, PhD San Diego, California
 Janine Jagger, MPH, PhD Charlottesville, Virginia
 William R. Jarvis, MD Atlanta, Georgia
 Douglas S. Kernodle, MD Nashville, Tennessee
 Robert H. Latham, MD Nashville, Tennessee
 Lewis B. Lefkowitz, MD Nashville, Tennessee
 Hsieh-Shong Leu, MD, MSc Taipei, Taiwan
 Jack Levy, MD Brussels, Belgium
 Victor Lorian, MD Bronx, New York
 Dennis G. Maki, MD Madison, Wisconsin
 Professor Dr. Walter Marget Munich, Federal Republic of Germany
 William J. Martone, MD Bethesda, Maryland
 Allison McGeer, MD Toronto, Ontario, Canada
 John E. McGowan, Jr., MD Atlanta, Georgia
 Jonathan L. Meakins, MD, DSc Montreal, Quebec, Canada
 Raf Mertens, MD Brussels, Belgium
 Robert R. Muder, MD Pittsburgh, Pennsylvania
 Joseph M. Mylotte, MD, CIC Buffalo, New York
 Lindsay Nicolle, MD Winnipeg, Manitoba, Canada
 Juhani Ojajarvi, MD Helsinki, Finland
 Michael T. Osterholm, PhD, MPH Minneapolis, Minnesota
 Jan Evans Patterson, MD San Antonio, Texas
 Sindy M. Paul, MD Trenton, New Jersey
 Michael A. Pfaller, MD Iowa City, Iowa
 Samuel Ponce de Leon, MD, MSc Mexico City, Mexico
 Isaam Raad, MD Houston, Texas
 Manfred L. Rotter, MD, DipBact Vienna, Austria
 Theodore Sacks, MD Jerusalem, Israel
 William E. Scheckler, MD Madison, Wisconsin
 Kent Sepkowitz, MD New York City, New York
 Denis Spelman, MD Prahran Victoria, Australia
 Michael L. Tapper, MD New York, New York
 Clyde Thornsberrry, PhD Brentwood, Tennessee
 Professor Leonid P. Titov Minsk, Republic of Belarus
 Timothy R. Townsend, MD Millwood, Virginia
 Antoni Trilla, MD, PhD Barcelona, Spain
 Professor Wang Shu-Qun Beijing, People's Republic of China
 J. John Weems, Jr., MD Greenville, South Carolina
 Robert A. Weinstein, MD Chicago, Illinois
 Professor Dr. W. Weuffen Greifswald, Federal Republic of Germany
 Sergio B. Wey, MD São Paulo, Brazil
 Rebecca Wurtz, MD Evanston, Illinois

SLACK Incorporated

6900 Grove Road
 Thorofare, New Jersey 08086
 (609) 848-1000

Vice President/Group Publisher

Richard N. Roash

Publisher

John C. Carter

Editorial Director

Jennifer Kilpatrick

Production Editor

Shirley P. Strunk, ELS

Assistant Editor

Eileen C. Anderer

Circulation Manager

Lester J. Robeson, CCCC

Production Director

Christine Malin

Production Coordinator

Joanne Patterson

Publishing Director/ Advertising

Wayne McCourt

Pharmaceutical Group Sales Director

Michael LoPresti

Advertising Sales Representative

Jennine Kane

Classified/Recruitment Sales Manager

Michele Burch

What do you mean I'm *not* protected?

If you are in the habit of applying hand cream after using a Chlorhexidine Cluconate (CHC) handwash, you may actually be losing your protection! A recent study* confirms that residual CHC can be neutralized by anionic hand creams.

Introducing.. **Lotion Soft@ Skin Conditioner**, a nonionic skin care lotion compatible with any CHG handwashing product. **Lotion Soft@ Skin Conditioner** contains emollients and moisturizers, which are soothing and last through several handwashes.

When you scrub with CHC for antimicrobial protection, you should be using a compatible product for skin conditioning. Try new **Lotion Soft@ Skin Conditioner**. It will not interfere with the cumulative effects of CHG.

Contact your local Calgon Vestal Healthcare Market Specialist or call toll-free 1-800-325-8005 to find out about new CHG compatible **Lotion Soft@ Skin Conditioner**.

Lotion Soft Skin Conditioner
The compatible companion



DIVISION OF CALGON CORPORATION
SUBSIDIARY OF **MERCK**
& CO., INC.

Box 147, ST. LOUIS, MO 63166

1-800-325-8005

See us at Booth "A" APIC

*test data on file