

April 1950 ✓

*Howarth*  
Vol. LXIV. No. 4

# The Journal of Laryngology and Otology

EDITED BY  
WALTER HOWARTH

WITH THE ASSISTANCE OF  
G. H. BATEMAN    R. G. MACBETH    V. E. NEGUS  
R. SCOTT STEVENSON    J. F. SIMPSON

## Contents

TUBERCULOUS LARYNGITIS TREATED BY STREPTOMYCIN	WILLIAM MCKENZIE
THE DECIBEL, THE PHON AND THE SONE . . . .	A. TUMARKIN
ENDOSCOPY IN THE MIDDLE EAST . . . . .	E. H. R. ALTOUNYAN
CLINICAL RECORD—	
CHONDROMA OF THE VOCAL CORD . . . . .	D. BROWN KELLY
CLINICAL NOTE—	
POINTS CONCERNING THE POSTERO-SUPERIOR FENESTRATION APPROACH . . . . .	C. A. HUTCHINSON
SOCIETIES' PROCEEDINGS—	
THE SCOTTISH OTOLOGICAL AND LARYNGOLOGICAL SOCIETY . . . . .	
ABSTRACTS—	
THE EAR	MISCELLANEOUS
THE OESOPHAGUS	
GENERAL NOTES	

London

Headley Brothers

109 Kingsway, W.C.2

Monthly, 7/6 net post free

Annual Subscriptions £3/3/0 net

# The Journal of Laryngology and Otology

(Founded in 1887 by MORELL MACKENZIE and NORRIS WOLFENDEN)

EDITED BY

WALTER HOWARTH

WITH THE ASSISTANCE OF

G. H. BATEMAN      R. G. MACBETH      V. E. NEGUS  
R. SCOTT STEVENSON      J. F. SIMPSON


1. Original Articles are accepted on the condition that they have not been published elsewhere.
2. Manuscripts should be typewritten, on one side only of the paper, and well spaced.
3. Galley proofs and engraver's proofs of illustrations are sent to the author. Corrections, which should be kept to a minimum, must be clearly marked, and no additional matter added.
4. Blocks illustrating articles are normally paid for by the *Journal*. Authors may, however, be required at the Editor's discretion, to contribute towards the cost of these in cases where this is particularly heavy.
5. Orders for reprints should be sent when returning galley proofs, and for this purpose special forms are supplied.
6. Authors of original communications on Oto-Laryngology in other journals are invited to send a copy, or two reprints, to the *Journal of Laryngology*. If they are willing, at the same time, to submit their own abstract (in English, French, Italian, or German) it will be welcomed.
7. Editorial communications may be addressed to THE EDITOR, *Journal of Laryngology*, c/o HEADLEY BROTHERS, 109 Kingsway, London, W.C.2.
8. The annual subscription is three guineas sterling, post free, and is payable in advance.
9. Single copies will be on sale at 7s. 6d. each; copies of parts up to Vol. LXIII may be purchased at 4s. each.
10. All subscriptions, advertising and business communications should be sent to the publishers, HEADLEY BROTHERS, 109 Kingsway, London, W.C.2.

#### *United States of America*

Orders for this *Journal* may be sent either through a local bookseller, or to Messrs. G. E. STECHERT & Co., 31-33 East 10th Street, New York, or they may be sent direct to the publishers, HEADLEY BROTHERS, 109 Kingsway, London, W.C.2, England.

Please mention *The Journal of Laryngology* when replying to advertisements

# THE AMPLIVOX AUDIOMETER

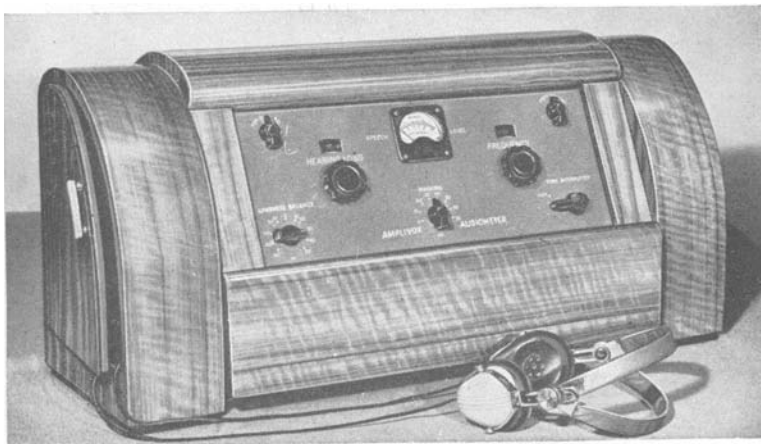

## *The Basic Instrument of Modern Otology*

### NEW TESTS NOW POSSIBLE

Speech-loss measurement in decibels now obtainable through dynamic microphone and speech input meter.

Loudness balance control gives measurement of the recruitment factor.

Input for group-test equipment and gramophone.

### CONSISTENT ACCURACY OF RESULTS

Eleven exact test frequencies 125-12,000 c.p.s.

Voltage compensation ensures that signal intensity does not vary should mains voltage do so.

### CALIBRATED MASKING TONE

Masking intensity varies equally with normal hearing acuity over range 125-4,000 c.p.s., permitting accurate masking control. Calibrated in decibels.

### SIMPLICITY OF OPERATION

Twin matched headphones (on double headband) for all air conduction tests; bone conductor on single headband, or interchangeable with one 'phone.


Hearing Loss dial calibrated in 5 dB steps from minus 10 dB to plus 100 dB.

Same figures on dial are read for air and bone conduction, and for all frequencies.

*Full details are available from the manufacturer, who will gladly arrange demonstrations, if required.*

**AMPLIVOX LTD., 2 BENTINCK ST., LONDON, W.1. (Welbeck 2591)**


Please mention *The Journal of Laryngology* when replying to advertisements

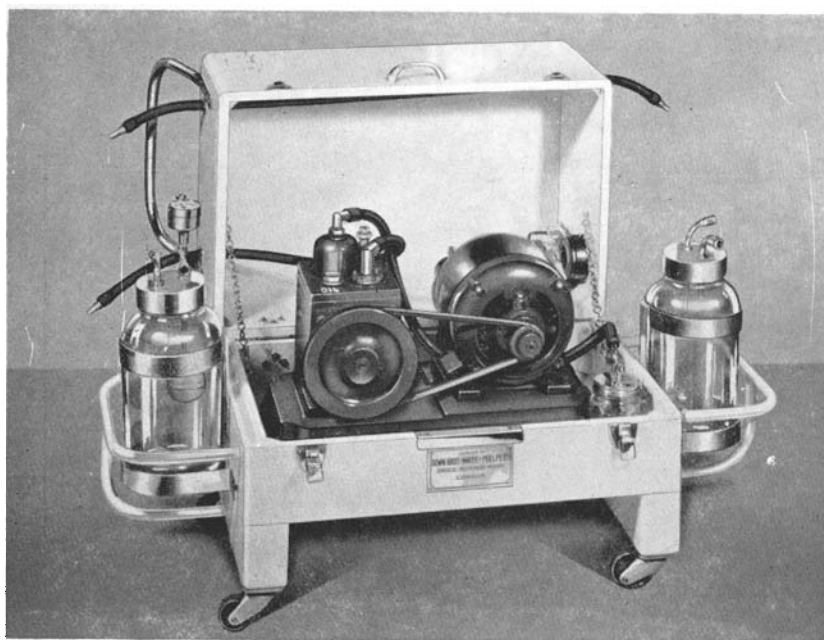

ELECTRIC

“Stand by” Foot  
Model, in case of  
electric supply  
failure. £3 3s. 0d.

*(Pump and Bottles)  
(Suction Tube extra)*

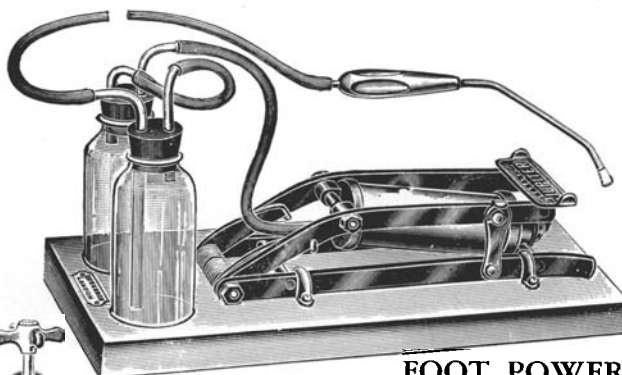

FOOT POWER

SUCTION  
APPARATUS



Or  
WATER

Particulars on application

**DOWN BROS. & MAYER & PHELPS Ltd.**

Showrooms: 32/34 NEW CAVENDISH ST., LONDON, W.1

Telephone:  
WELBECK 3764

DOWN BROS. AND MAYER & PHELPS HAVE AMALGAMATED.  
THE PERSONAL MANagements REMAIN AS HERETOFORE.

Please mention *The Journal of Laryngology* when replying to advertisements

**PRESCRIBE THE EASY EFFECTIVE METHOD**


When spraying, the patient can hold his head in a natural position, yet the solution spreads throughout the nasal cavity, assuring thorough treatment. Effective dropper-application, on the other hand, requires a complicated posture technique which patients are apt to neglect in home treatment.



**DeVilbiss  
ATOMIZERS**




**DROPPER ?**



**ATOMIZER ?**


These illustrations, which are based on X-ray research, clearly demonstrate the advantages of the atomizer as compared with the dropper  
**The AEROGRAPH Co., Ltd., Lower Sydenham, London, S.E.26**  
*Sole Distributors of DeVilbiss Products in the United Kingdom.*  
 Telephones : Sydenham 6060—8 Lines.

CVS—225

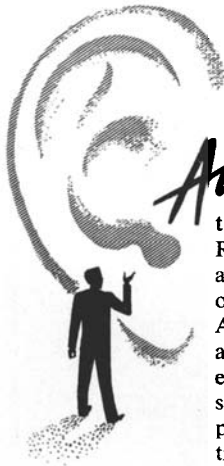

*Aurally Speaking*

In the measurement of hearing loss, the Pure Tone Audiometer, TF 895, conforms to the specification of the Committee on Electro-Acoustics appointed by the Medical Research Council. Each instrument is individually calibrated against N.P.L. determinations and will therefore provide a reading, on a given patient, comparable with that of any other Marconi Audiometer. Orally instructed through a crystal microphone and high-fidelity earphones, the patient responds via a signal lamp built-in to the instrument panel. Please ask for further information of this improved aid to audiometry.

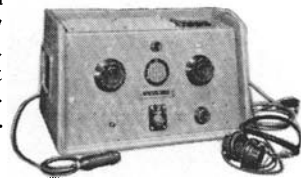

Type TF 895

**PURE TONE Audiometer**

**MARCONI INSTRUMENTS LTD.**

ST. ALBANS, HERTFORDSHIRE • Telephone : St. Albans 6161/5  
 Northern Office : 30 Albion Street, Hull. Western Office : 76 Portview Road, Avonmouth. Midland Office :  
 19 The Parade, Leamington Spa. Southern Office and Showrooms : 109 Eaton Square, London, S.W.1.

Please mention *The Journal of Laryngology* when replying to advertisements



## THE S.D. PORTABLE AUDIOMETER A.C./D.C.

**T**HIS genuinely portable Audiometer, built into a strong carrying case, offers great accuracy combined with convenience in use.

It incorporates an extremely stable beat frequency oscillator giving a continuous range of frequency, and a built-in valve voltmeter not only allows accurate zero setting of frequency but ensures a constant result whatever the conditions of voltage or of valve life.

A crystal microphone and amplifier give excellent speech reproduction and in addition enable speech level tests to be made. A masking note of mixed low frequency and a manual mute are also provided.

Our Peepshow for testing the hearing of young children can be used with this Audiometer.

**ALFRED PETERS & SONS LTD.**  
FARGATE HOUSE · SHEFFIELD 1

Please mention *The Journal of Laryngology* when replying to advertisements



## THE SD/2 AUDIOMETER

**T**HIS instrument offers not only great accuracy but incorporates some unique features, which allow a most comprehensive range of tests to be made and ensures a constant result under all conditions of voltage and valve life.

It includes among many facilities an automatic interruptor circuit, as well as a continuous tone: twin matched earphones allowing the test and masking tones to be switched to either ear, while a balance control enables the response of each ear to be matched simultaneously.

A built-in crystal microphone and amplifier give excellent speech reproduction and allow speech level tests to be made, while the built-in meter and cathode ray tube ensure continuing accuracy of frequency and output.

Our Peepshow for testing young deaf children may be used with this Audiometer.

**ALFRED PETERS & SONS LTD.**  
FARGATE HOUSE · SHEFFIELD 1

Please mention *The Journal of Laryngology* when replying to advertisements

# CONTENTS

	PAGE
TUBERCULOUS LARYNGITIS TREATED BY STREPTOMYCIN. William McKenzie (London) . . . . .	167
THE DECIBEL, THE PHON AND THE SONE. A. Tumarkin (Liverpool)	178
ENDOSCOPY IN THE MIDDLE EAST. E. H. R. Altounyan (Aleppo, Syria) . . . . .	189
CLINICAL RECORD—	
Chondroma of the Vocal Cord. D. Brown Kelly (Glasgow)	195
CLINICAL NOTE—	
Points concerning the Postero-superior Fenestration Approach. C. A. Hutchinson (Salisbury) . . . . .	198
SOCIETIES' PROCEEDINGS—	
The Scottish Otological and Laryngological Society . . . . .	203
ABSTRACTS—	
Ear . . . . .	215
Interpretation of Hearing Tests. Stacy R. Guild; Evaluation of Dizziness. David D. DeWeese.	
Œsophagus . . . . .	216
Diagnosis of Lesions near the Cardia. John H. Fitzgibbon.	
Miscellaneous . . . . .	216
Anticoagulant Therapy in Surgery. Geza De Takats; Laryngeal versus Gastric Cultures in the Detection of Tubercle Bacilli. M. Duggan and Laura Delamater.	
GENERAL NOTES . . . . .	218

For Advertisement space in this Journal apply to :  
**HEADLEY BROTHERS, 109 Kingsway, London, W.C.2**

---

Please mention *The Journal of Laryngology* when replying to advertisements