

The Journal of Laryngology and Otology

EDITED BY
WALTER HOWARTH

WITH THE ASSISTANCE OF
G. H. BATEMAN R. G. MACBETH V. E. NEGUS
R. SCOTT STEVENSON J. F. SIMPSON

Contents

THE MORGAGNI-STEWART-MOREL SYNDROME AND THE OTOLOGIST	C. A. HUTCHINSON
SPEECH AUDIOMETRY IN THE ASSESSMENT OF DEAFNESS	E. D. D. DICKSON and D. L. CHADWICK
PERCEPTIVE DEAFNESS ASSOCIATED WITH SEVERE NEONATAL JAUNDICE	NORMAN CRABTREE and JOHN GERRARD
RESIDUAL OSTEITIS OF THE ALVEOLUS OF THE MAXILLA AS A CAUSE OF FACIAL PAIN	PHILIP S. MEYRICK and LESLIE S. MANION
CLINICAL RECORDS—	
CARCINOMA OF THYROID WITH WIDESPREAD METASTASES AND UNUSUAL SYMPTOMA- TOLOGY	J. B. CAVENAGH and W. H. McMENEMEY
SPONTANEOUS RUPTURE OF THE SIGMOID SINUS IN A CASE OF MASTOIDITIS	JOHAN W. MORGANTHAL
CEREBRAL HÆMATOMA COMPLICATING EXTRA- DURAL ABSCESS	L. F. DAY
SOCIETIES' PROCEEDINGS—	
THE NORTH OF ENGLAND OTO-LARYNGOLOGICAL SOCIETY	
ABSTRACTS—	
THE EAR	THE OESOPHAGUS
THE NOSE	MISCELLANEOUS
THE LARYNX	
REVIEW	

London

Headley Brothers

109 Kingsway, W.C.2

Monthly, 7/6 net post free

Annual Subscriptions £3/3/0 net

The Journal of Laryngology and Otology

(Founded in 1887 by MORELL MACKENZIE and NORRIS WOLFENDEN)

EDITED BY

WALTER HOWARTH

WITH THE ASSISTANCE OF

G. H. BATEMAN R. G. MACBETH V. E. NEGUS
R. SCOTT STEVENSON J. F. SIMPSON

1. Original Articles are accepted on the condition that they have not been published elsewhere.
2. Manuscripts should be typewritten, on one side only of the paper, and well spaced.
3. Galley proofs and engraver's proofs of illustrations are sent to the author. Corrections, which should be kept to a minimum, must be clearly marked, and no additional matter added.
4. Blocks illustrating articles are normally paid for by the *Journal*. Authors may, however, be required at the Editor's discretion, to contribute towards the cost of these in cases where this is particularly heavy.
5. Orders for reprints should be sent when returning galley proofs, and for this purpose special forms are supplied.
6. Authors of original communications on Oto-Laryngology in other journals are invited to send a copy, or two reprints, to the *Journal of Laryngology*. If they are willing, at the same time, to submit their own abstract (in English, French, Italian, or German) it will be welcomed.
7. Editorial communications may be addressed to THE EDITOR, *Journal of Laryngology*, c/o HEADLEY BROTHERS, 109 Kingsway, London, W.C.2.
8. The annual subscription is three guineas sterling, post free, and is payable in advance.
9. Single copies will be on sale at 7s. 6d. each; copies of parts up to Vol. LXIII may be purchased at 4s. each.
10. All subscriptions, advertising and business communications should be sent to the publishers, HEADLEY BROTHERS, 109 Kingsway, London, W.C.2.

United States of America

Orders for this *Journal* may be sent either through a local bookseller, or to Messrs. G. E. STECHERT & Co., 31-33 East 10th Street, New York, or they may be sent direct to the publishers, HEADLEY BROTHERS, 109 Kingsway, London, W.C.2, England.

Please mention *The Journal of Laryngology* when replying to advertisements

AMPLIVOX

Model 61*

AUDIOMETER



* An improved version of the famous Model 60

The Basic Instrument of Modern Otology

More compact than its predecessor the Amplivox Model 61 audiometer occupies minimum desk room and the control panel is at the eye level of the operator when seated. The cabinet has been made extremely robust and fitted with a lock-up drawer to hold accessories and prevent unauthorized use of the instrument.

The technical features of the Model 60 are retained.

- Eleven exact test frequencies 125-12,000 c.p.s.
- Simplified hearing loss dial. The same set of figures is read for both bone and air conduction at all frequencies, and for speech.
- Bone conduction tests can be made from 125-4,000 c.p.s.
- Masking Tone calibrated in decibels, permitting accurate control of masking.
- Double Air receivers enable test tones to be switched instantly from ear to ear
- Speech test circuit monitors speech level, permitting accurate measurement of hearing loss for speech.
- Loudness Balance Control establishes presence of recruitment in monaural deafness.
- Automatic voltage compensator.


Recruitment Test Set accessory establishes presence of recruitment by amplitude modulation, enabling each ear to be tested independently.

Speech Turntable and English-made Harvard Spondee records also available.

*Full details are available from the manufacturers
who will gladly arrange demonstrations if required*

AMPLIVOX LTD., 2 BENTINCK ST., LONDON, W.1 (Welbeck 2591)


Please mention *The Journal of Laryngology* when replying to advertisements

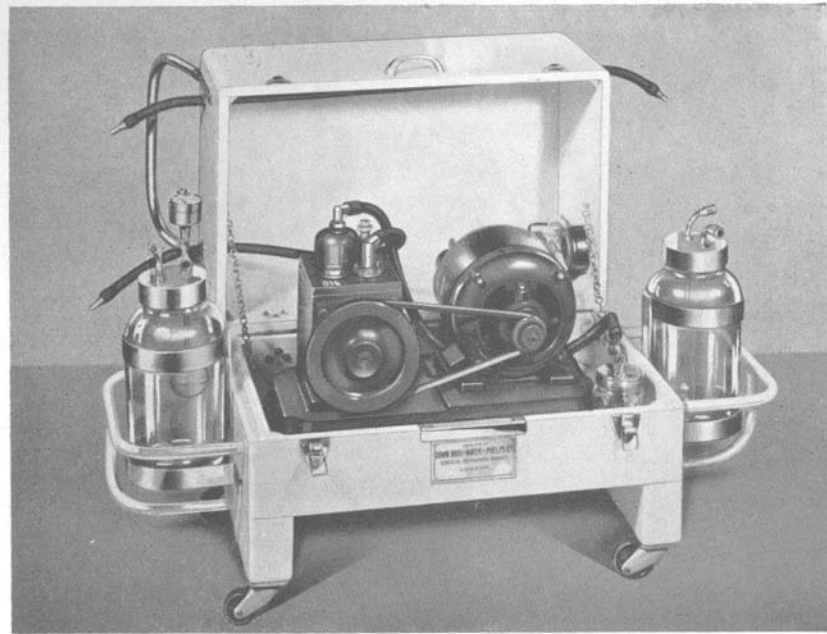

ELECTRIC

“Stand by” Foot
Model, in case of
electric supply
failure. £3 3s. 0d.

*(Pump and Bottles)
(Suction Tube extra)*

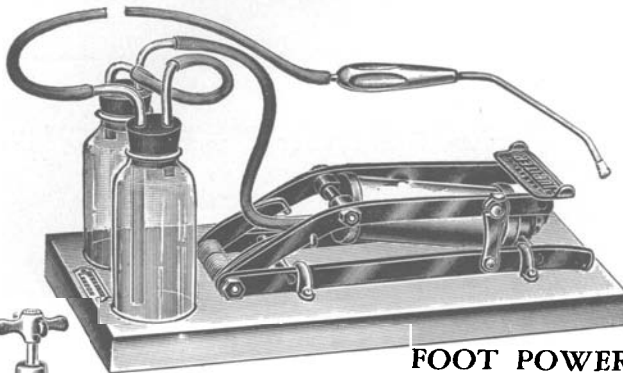

FOOT POWER

**SUCTION
APPARATUS**

Or
WATER

Particulars on application

DOWN BROS. & MAYER & PHELPS Ltd.

Showrooms: 32/34 NEW CAVENDISH ST., LONDON, W.1

Telephone:
WELBECK 3764

DOWN BROS. AND MAYER & PHELPS HAVE AMALGAMATED.
THE PERSONAL MANagements REMAIN AS HERETOFORE.

Please mention *The Journal of Laryngology* when replying to advertisements

PRESCRIBE THE EASY EFFECTIVE METHOD

When spraying, the patient can hold his head in a natural position, yet the solution spreads throughout the nasal cavity, assuring thorough treatment. Effective dropper-application, on the other hand, requires a complicated posture technique which patients are apt to neglect in home treatment.



DROPPER ?



ATOMIZER ?



**DeVilbiss
ATOMIZERS**

These illustrations, which are based on X-ray research, clearly demonstrate the advantages of the atomizer as compared with the dropper
The AEROGRAPH Co., Ltd., Lower Sydenham, London, S.E.26
Sole Distributors of DeVilbiss Products in the United Kingdom.
 Telephones: Sydenham 6060—8 Lines.

AMPLIVOX

Model 70

PORTABLE AUDIOMETER

Light . . . Simple . . . Exact



FOR RAPID AND ACCURATE HEARING TESTING AND SCREENING


This new audiometer enables accurate pure tone air conduction tests to be effected from 125-8,000 c.p.s. Light yet robust and extremely simple to operate, the Model 70 answers the demand of Otologists, Hospitals, Schools and Industry for an inexpensive but accurate audiometer where complete diagnostic features are not necessary.

Uniform zero reference level enables hearing loss control to be set at desired intensity for screening tests, and individual frequencies to be checked in succession without readjustment. A recent survey showed that 10 year old schoolchildren could be individually screened in this way in an average time of 2½ minutes per child. *Full air conduction tests down to threshold can be performed on the same instrument.*


The Model 70 operates on either A.C. or D.C. mains from 100 to 250 volts and the complete instrument weighs only 14 lbs. Price 80 guineas, weatherproof cover 1 guinea.

AMPLIVOX LTD., 2 BENTINCK STREET, LONDON, W.1. (WELbeck 2591/4)

Please mention *The Journal of Laryngology* when replying to advertisements

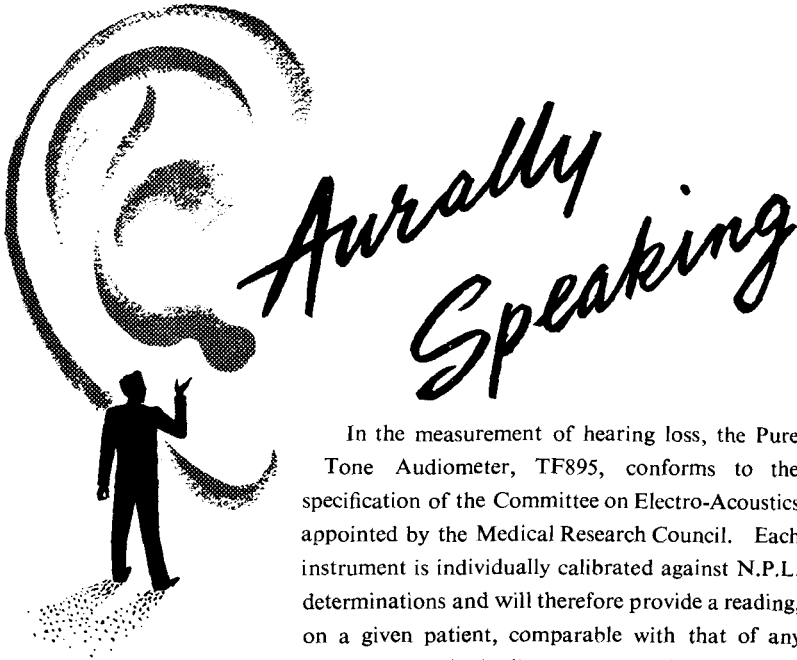

In the measurement of hearing loss, the Pure Tone Audiometer, TF895, conforms to the specification of the Committee on Electro-Acoustics appointed by the Medical Research Council. Each instrument is individually calibrated against N.P.L. determinations and will therefore provide a reading, on a given patient, comparable with that of any other Marconi Audiometer. Orally instructed through a crystal microphone and high-fidelity earphones, the patient responds via a signal lamp built-in to the instrument panel. Please ask for further information of this improved aid to audiometry.

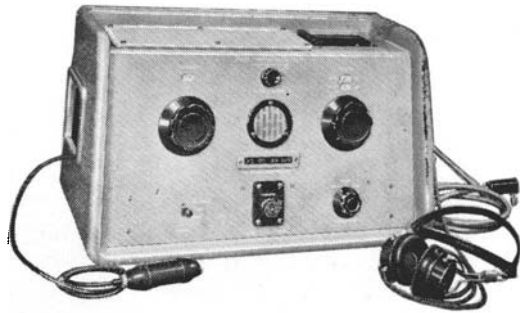

PURE TONE

AUDIOMETER

Type TF 895

MARCONI INSTRUMENTS LTD.

ST. ALBANS, HERTFORDSHIRE · Telephone: St. Albans 6161/5

Northern Office: 30 Albion Street, Hull. Western Office: 76 Portview Road, Avonmouth. Midland Office: 19 The Parade, Leamington Spa. Southern Office and Showrooms: 109 Eaton Square, London, S.W.1.

Please mention *The Journal of Laryngology* when replying to advertisements



A Significant Advance in AUDIOMETRIC TECHNIQUE


Produced as the result of consultations with Medical Authorities, both in this country and abroad, the Belclere A.2.A. Audiometer incorporates all the improvements rendered desirable in the light of practical experience.

Among other distinguishing features is the inclusion of dual calibration, with twin attenuators, for binaural recruitment tests. Provision is also made for gramophone recorded speech tests.

Write for our free, comprehensive brochure, "Modern Audiometric Technique". An authoritative work on the constructive and operative principles of modern Audiometers and their uses.

JOHN BELL & CROYDEN
Wigmore Street, London, W. 1
or Acoustic Instrument Works, Oxford

THE
Belclere
TYPE A.2.A.

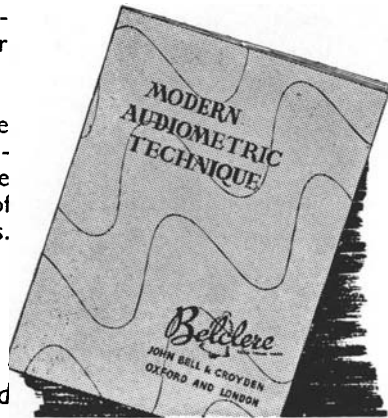

Please mention *The Journal of Laryngology* when replying to advertisements

CONTENTS

	PAGE
THE MORGAGNI-STEWART-MOREL SYNDROME AND THE OTOLOGIST. C. A. Hutchinson (Salisbury)	455
SPEECH AUDIOMETRY IN THE ASSESSMENT OF DEAFNESS. Air Commodore E. D. D. Dickson and Flight-Lieut. D. L. Chadwick	464
PERCEPTIVE DEAFNESS ASSOCIATED WITH SEVERE NEONATAL JAUNDICE. Norman Crabtree and John Gerrard (Birmingham)	482
RESIDUAL OSTEITIS OF THE ALVEOLUS OF THE MAXILLA AS A CAUSE OF FACIAL PAIN. Philip S. Meyrick and Leslie S. Manion (Pietermaritzburg, Natal)	507
CLINICAL RECORDS—	
Carcinoma of Thyroid with Widespread Metastases and Unusual Symptomatology. J. B. Cavenagh and W. H. McMenemey (Worcester)	517
Spontaneous Rupture of the Sigmoid Sinus in a Case of Mastoiditis. Johan W. Morganthal (East London, South Africa)	521
Cerebral Hæmatoma Complicating Extradural Abscess. L. F. Day (Hastings)	523
SOCIETIES' PROCEEDINGS—	
The North of England Oto-Laryngological Society	527
ABSTRACTS—	
Ear	537
Fenestration of the Internal Ear, with Analysis of 33 Cases. B. W. Tanton; On Antistin Therapy of the Ménière Symptom Complex. K. Burian; Bone Conduction in Otosclerosis. R. R. Woods; Endolymphatic Hydrops without Vertigo; Its Differential Diagnosis, and Treatment. Henry L. Williams, Bayard T. Horton and Lois A. Day; The Management of Tinnitus. Victor Goodhill; On Subjective Noise in Labyrinthectomy Patients. F. Neuberger.	
Nose	539
Dental Injuries following Radical Surgery on the Maxillary Sinus. Gunnar Martensson; The Management of Malignancy of the Maxillary Sinus. Arnold A. Grossman, W. Allan Donnelly and Maurice F. Saitman.	
Larynx	541
The Respiratory Function in Laryngectomized Patients. Rutger Heyden.	
Œsophagus	541
Œsophageal Hiatal Hernia. Thomas A. Shallow, F. Johnson Putney and Kenneth E. Fry.	
Miscellaneous	541
Para-aminosalicylic Acid with Streptomycin in Tuberculosis. W. Anderson, M. G. W. Jansen and C. A. Wicks; Pathologico-Anatomical Investigations on Sulphonamide-Treated Otogenous Meningitis. F. Krejci; Tobacco Smoking as a Possible Etiologic Factor in Bronchiogenic Carcinoma: A Study of 684 Proved Cases. Ernest L. Wynder and Everts A. Graham; Cancer and Tobacco Smoking: A Preliminary Report. Morton L. Levin, Hymna Goldstein and Paul R. Gerhardt; Antihistaminic Drugs for Colds: Evaluation Based on a Controlled Study. Lt.-Col. R. J. Hoagland, Capt. E. N. Dietz, Lt. P. W. Myers and Lt. H. C. Cosand; Antihistaminic Agents and Ascorbic Acid in the Early Treatment of the Common Cold. Donald W. Cowan and Harold S. Diehl; Histological Reactions to Injections of Procaine Penicillin in Oil. Peter Story; Secondary Bronchial Carcinoma Simulating a Strangulated Femoral Hernia. E. Wilson Hall, A. Geoffrey Shera and E. Owen Fox; The New Oto-Laryngo- logical Department of the University Hospital, Upsala, Sweden. C. O. Nylén; Aerosol Therapy for Lung Disease. H. K. Christie, M. Aronovitch and J. F. Meakins.	
REVIEW	546